


Surveyor Review

REVIEW STATION FOR SURVEYOR TELEMETRY CENTRAL 12-LEAD ECG DATA

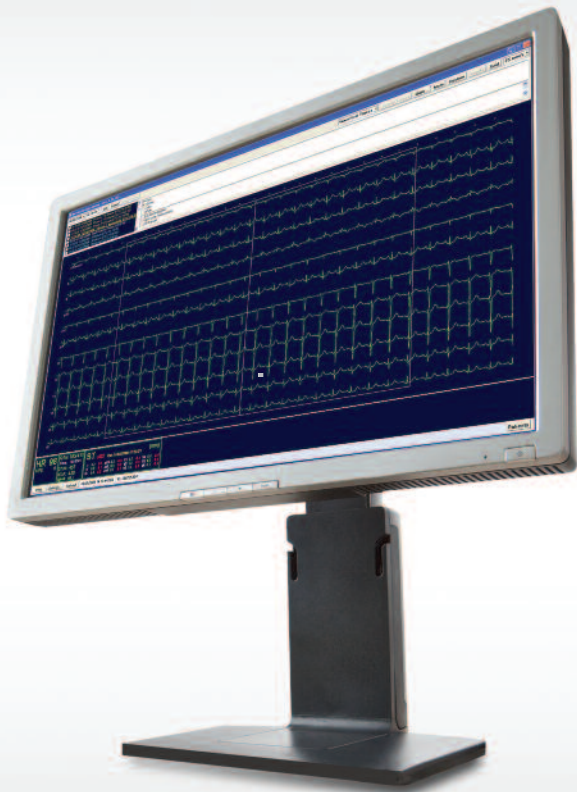

PRODUCT FEATURES

- **Surveyor™ Telemetry Central Data Online Review**

Network Surveyor Review stations to the Surveyor Telemetry Central system database with administrator-authorized permissions to remotely review in-progress patient monitoring data.

- **Surveyor Telemetry Central Data Archive Review**

Standalone Surveyor Review station can be used to review Surveyor Central monitoring data archived to media or a networked location. Surveyor Review is available as a turnkey system or software kit.

- **Review and Filter Stored Events**

Alarm events can be filtered, retrieved, and reviewed by hierarchy and groups. A simple mouse click on any event immediately displays the ECG waveform in a user-defined display format.

- **Review and Print Graphical and Tabular Trends**

Multiple user-selectable trend display selections for quick comparison of related events and ECG changes.

- **Simple Monitoring Data Navigation**

Full-disclosure review through entry of a date and time or a mouse click on a trend point; beat-by-beat ECG review with simple forward and reverse navigation tools.

- **12-Lead ECG Interpretation**


Printed 12-lead ECGs can include the VERITAS™ 12-lead resting ECG interpretation and global measurements.

- **Print and Export 12-Lead ECG**

Ability to change ECG format settings and number of rhythm leads. 12-lead ECG interpretation feature supports export to E-Scribe™ data management system.

12-LEAD telemetry monitoring review

 **Mortara**

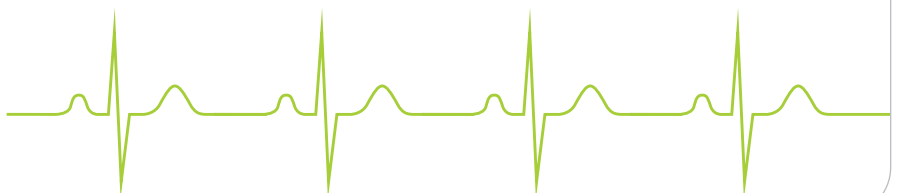

**MORTARA INSTRUMENT, INC.**

7865 North 86th Street
Milwaukee, WI 53224
U.S.A.

Tel: 414.354.1600
Tel: 800.231.7437
Service: 888.MORTARA
Fax: 414.354.4760

MORTARA RANGONI EUROPE, SRL

(European Headquarters)
Via Cimarosa 103/105
40033 Casalecchio di Reno (BO)
Italy
Tel: +39.051.298.7811
Fax: +39.051.613.3582

www.mortara.com

ISO 13485 CERTIFIED

WARRANTY + SERVICE

Mortara Instrument is committed to the highest level of customer support. Please contact us for the program which will be best suited for your needs.

**SURVEYOR™ REVIEW**

FEATURE	SPECIFICATIONS*
INSTRUMENT TYPE	Central Station Monitoring Review
CPU	Pentium IV (minimum)
OPERATING SYSTEM/RAM	Microsoft® Windows™ XP Professional with 512MB (minimum), Windows Vista Business with 1GB (minimum) and SPI, or Windows 7 32-bit with 1GB (minimum)
VIDEO RESOLUTION	1024 x 720 (minimum)
TRACES PER PATIENT	Up to 12 simultaneously
DISPLAY SPEED	5, 10, 25, or 50 mm/s
ECG SENSITIVITY	5, 10, 20, or 40 mm/mV
TRENDS	Up to 8 tabular or graphic
TREND DURATION PER DISPLAY SCREEN	3, 6, 12, and 24 hour
FULL-DISCLOSURE DISPLAY DURATION	Dependent on screen resolution, number of traces, and display speed; typically more than 1 hour per display screen
REVIEW METHOD	By event or by graphical trend
PRINTER COMPATIBILITY	Windows compatible, fully tested with HP 4000 series laser printer and PCL5 drivers; 1200 x 1200 dpi; 55 ppm max
PRINTOUT TYPES	Rhythm, 12-lead ECG, ST report, and trends
12-LEAD ECG PRINTOUT FORMATS	6x2, 4x3+1, 4x3+3, 4x3+1+P at 25 or 50 mm/s
PAPER TYPES	A4 and letter

*Specifications subject to change without notice.

E-Scribe™, Surveyor™, and VERITAS™ are trademarks of Mortara Instrument, Inc.

Microsoft® and Windows™ are trademarks or registered trademarks of Microsoft Corp.